


# PYROTHERM CCS 130

## Compact infrared calibration source/black body

### Overview

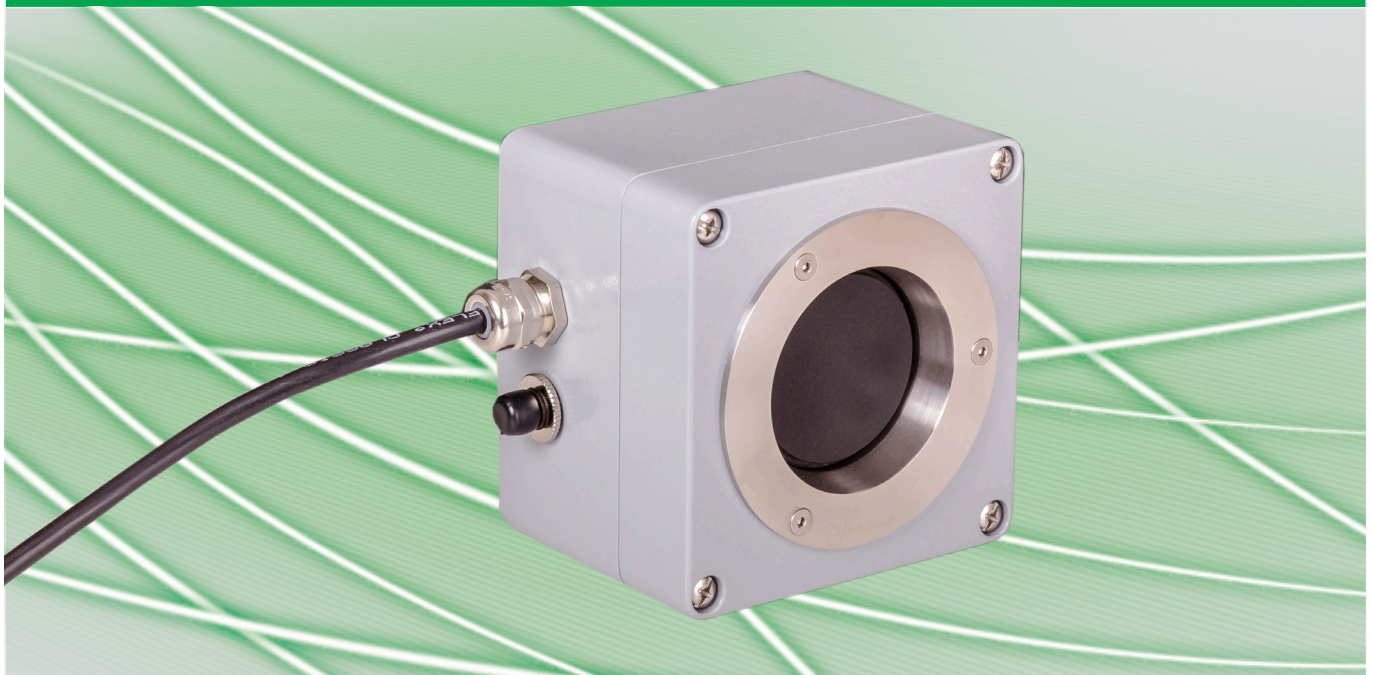

### Description

The calibration source PYROTHERM CCS 130 is used for calibration and examination of pyrometers and infrared cameras. The temperature is set ex-works and is between 30 °C and 130 °C. A robust housing enables the use even in harsh environments. The radiator surface has a high emissivity of 0.98. A precise temperature control guarantees the high precision and stability of the device.

### Technical data

Radiator temperature	30 °C to 130 °C (adjustable in steps of 1 °C at the factory)
Aperture diameter	55 mm
Emissivity <sup>1</sup>	0.98 ± 0.01
Measurement uncertainty <sup>1</sup>	0.5 K
Reproducibility	0.2 K
Control stability	0,2 K
Controler	PID
Heat up time	between 5 and 20 minutes
Connections	– 4-pin connection cable 5 m (power supply, input RUN, output READY) – service interface
Operating temperature	0 °C to 40 °C <sup>2</sup>
Storage temperature	–20 °C to 70 °C
Dimensions W × H × D	120 × 120 × 90 [mm]
Weight	1.8 kg
Power supply	24 V DC, 1 A

<sup>1</sup> For 8 µm to 14 µm. <sup>2</sup> Maximum operating temperature for radiator temperature < 45 °C: Radiator temperature minus 5 °C.

Technische Änderungen vorbehalten. Technical details are subject to change. 07.06.21



Phone: +49 351 896 74-0  
 Fax: +49 351 896 74-99  
 Email: info@dias-infrared.de  
 Internet: www.dias-infrared.com

DIAS Infrared GmbH  
 Pforzheimer Straße 21  
 01189 Dresden  
 Germany